

# How to remotely retrieve measurements with an SDS X and XE series of Oscilloscope

October 23, 2017

The command sequence for returning measurements with a SIGLENT SDS X and XE series of oscilloscopes is as follows:

MEAD <type>, <source> Activate measurement type

Where <type> = {PHA, FRR, FRF, FFR, FFF, LRR, LRF, LFR, LFF}

The PHA is phase, the others are the same as the specified type of the instruments delay measure in the SDS programming guide.

<source> = {C1-C2, C1-C3, C1-C4, C2-C3, C2-C4, C3-C4}

<source>:MEAD? <type> Return measurement data

Where <source> = {C1-C2, C1-C3, C1-C4, C2-C3, C2-C4, C3-C4}

<type> = {PHA, FRR, FRF, FFR, FFF, LRR, LRF, LFR, LFF}


The PHA is phase, the others are the same as the specified type of the instruments delay measure in the SDS programming guide.

The following example shows the command sequence to enable phase measurements between CH1 and CH2 on an SDS1202X Oscilloscope.


**NOTE:** The SDS1202X was set to default factory settings, CH2 was activated manually, and 2 sine waves with different phases were used as inputs to either channel.

The commands were sent using NI-MAX VISA Test Panel.

Here is the default display. Note, there are no measurements active on the display.

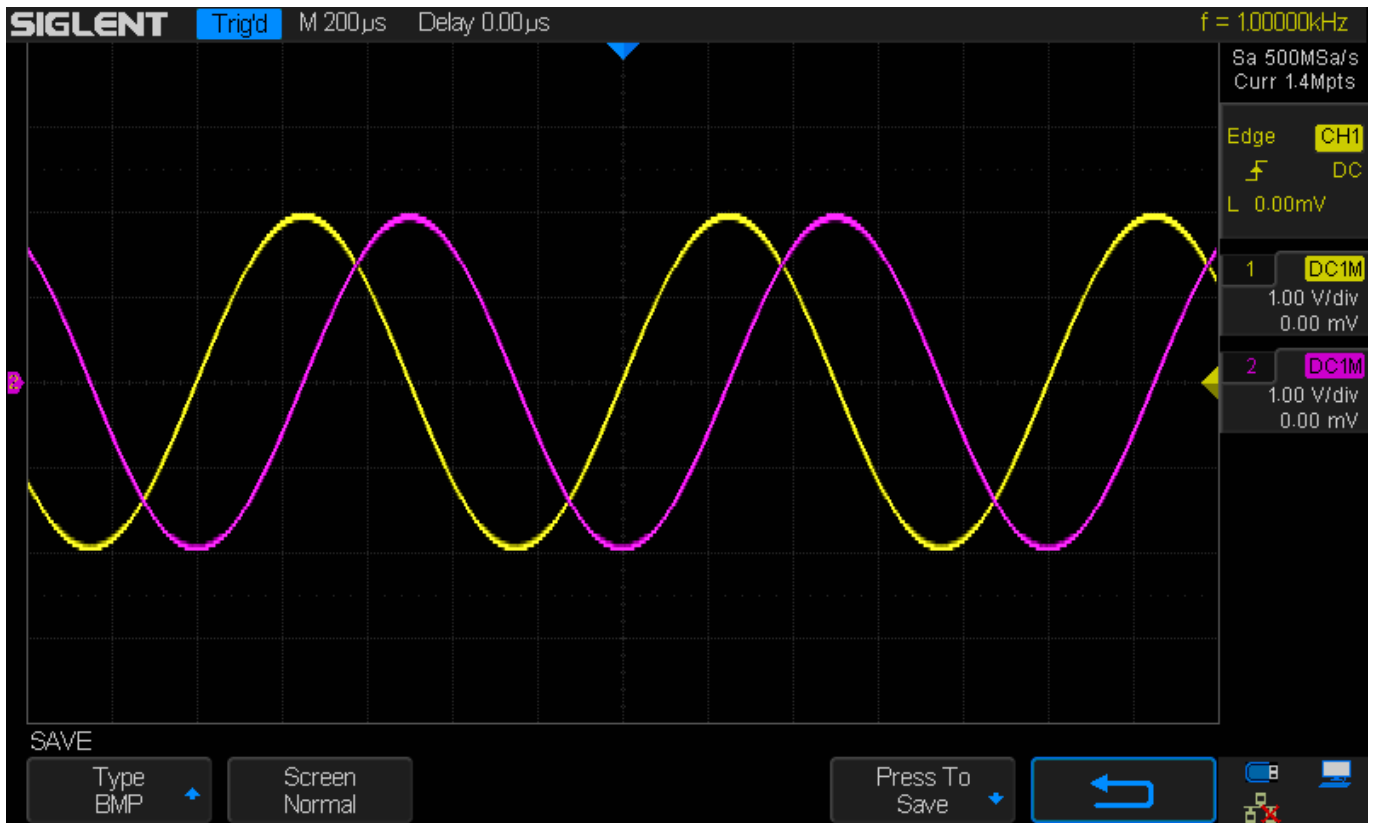

**Step 1:** Send "MEAD PHA,C1-C2" to activate phase measurements between CH1 and CH2.

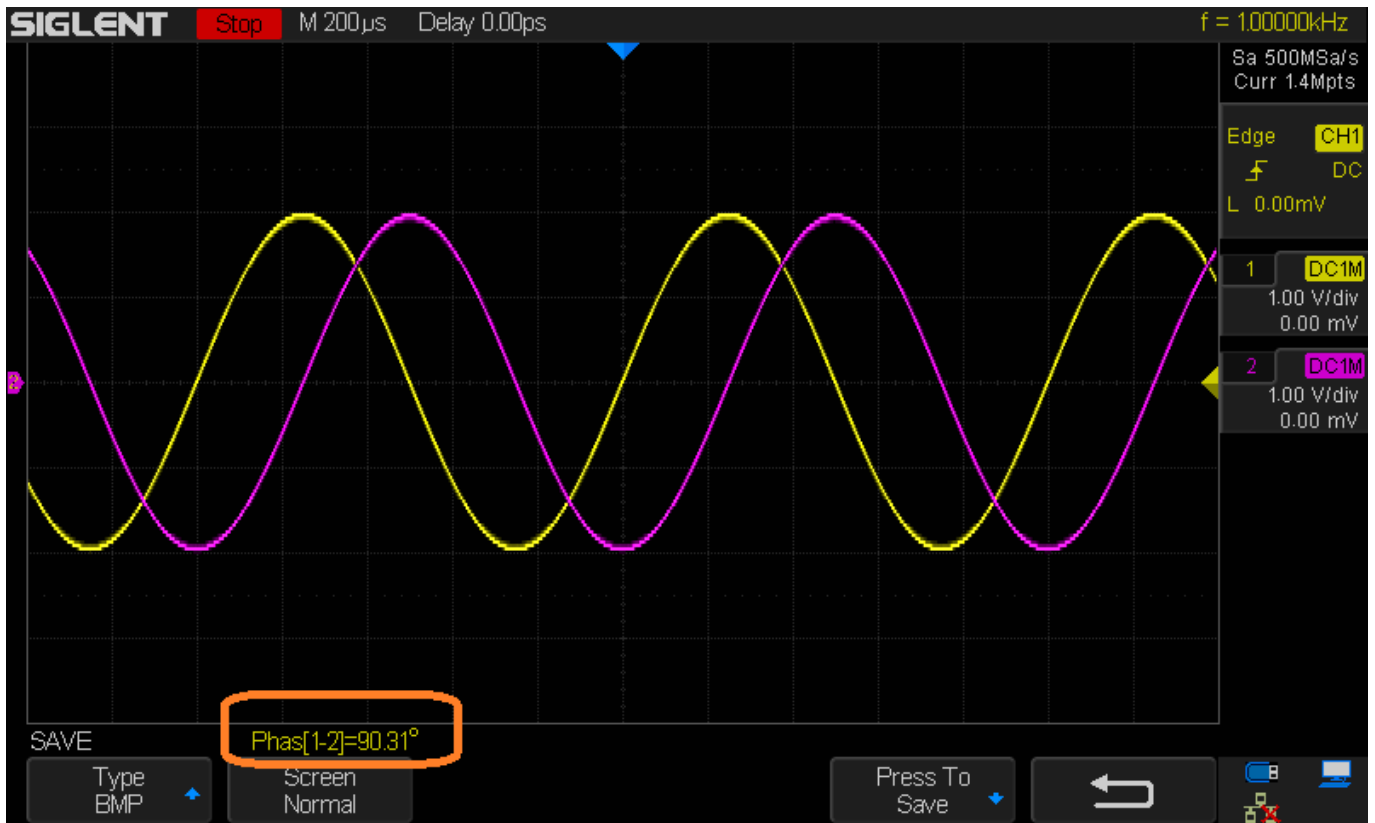

**Step 2:** Send "C1-C2:MEAD? PHA" to activate phase measurements between CH1 and CH2.



### **North American Headquarters**

SIGLENT Technologies NA  
6557 Cochran Rd Solon, Ohio 44139  
Tel: 440-398-5800  
Toll Free: 877-515-5551  
Fax: 440-399-1211  
[info@siglent.com](mailto:info@siglent.com)  
[www.siglentamerica.com/](http://www.siglentamerica.com/)

### **European Sales Offices**

SIGLENT TECHNOLOGIES GERMANY GmbH  
Staetzlinger Str. 70  
86165 Augsburg, Germany  
Tel: +49(0)-821-666 0 111 0  
Fax: +49(0)-821-666 0 111 22  
[info-eu@siglent.com](mailto:info-eu@siglent.com)  
[www.siglenteu.com](http://www.siglenteu.com)

### **Asian Headquarters**

SIGLENT TECHNOLOGIES CO., LTD.  
Blog No.4 & No.5, Antongda Industrial Zone,  
3rd Liuxian Road, Bao'an District,  
Shenzhen, 518101, China.  
Tel: + 86 755 3661 5186  
Fax: + 86 755 3359 1582  
[sales@siglent.com](mailto:sales@siglent.com)  
[www.siglent.com/ens](http://www.siglent.com/ens)